

# REPORT DOCUMENTATION PAGE

Form Approved  
OMB No. 0704-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.

|  |   |  |   |  |
|--|---|--|---|--|
| 1. AGENCY USE ONLY (Leave blank)   |   | 2. REPORT DATE   | 3. REPORT TYPE AND DATES COVERED<br>FINAL                                 |  |
| 4. TITLE AND SUBTITLE<br>FY92-93 HBCU/MI Instrumentation for the Pulsed Power and Plasma Sciences Laboratory at the University of New Mexico |   |  | 5. FUNDING NUMBERS<br><del>XXXXXX</del><br>4276/AS<br>62228D              |  |
| 6. AUTHOR(S)<br>Professor Schamiloglu  |   |  |   |  |
| 7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES)<br>University of New Mexico<br>Albuquerque, NM 87131-1356                                 |   |  | 8. PERFORMING ORGANIZATION<br>REPORT NUMBER<br><br>AFOSR-TR- 95 0165      |  |
| 9. SPONSORING MONITORING AGENCY NAME(S) AND ADDRESS(ES)<br>AFOSR/NE<br>110 Duncan Avenue Suite B115<br>Bolling AFB DC 20332-0001             |   |  | 10. SPONSORING MONITORING<br>AGENCY REPORT NUMBER<br><br>F49620-93-1-0585 |  |
| 11. SUPPLEMENTARY NOTES  |   |  |   |  |
| 12a. DISTRIBUTION AVAILABILITY STATEMENT<br><br>APPROVED FOR PUBLIC RELEASE: DISTRIBUTION UNLIMITED  |   |  | 12b. DISTRIBUTION CODE  |  |
| 13. ABSTRACT<br><br>SEE FINAL REPORT ABSTRACT  |   |  |   |  |
| 14. SUBJECT TERMS  |   |  | 15. NUMBER OF PAGES   |  |
|  |   |  | 16. PRICE CODE  |  |
| 17. SECURITY CLASSIFICATION<br>OF REPORT<br>UNCLASSIFIED   | 18. SECURITY CLASSIFICATION<br>OF THIS PAGE<br>UNCLASSIFIED | 19. SECURITY CLASSIFICATION<br>OF ABSTRACT<br>UNCLASSIFIED | 20. LIMITATION OF ABSTRACT<br>UNCLASSIFIED                                |  |

DTIC  
ELECTE  
MAR 27 1995



**The University of New Mexico**

Department of Electrical and  
Computer Engineering  
Room 110, EECE Building  
Albuquerque, NM 87131-1356  
(505) 277-2436

ORIGINAL

**Final Technical Report Submitted to AFOSR:  
FY92-93 HBCU/MI Instrumentation for the  
Pulsed Power and Plasma Sciences Laboratory  
at the University of New Mexico  
(Grant AFOSR #F49620-93-1-0585)**

30 November 1994

---

Edl Schamiloglu, Associate Professor, Principal Investigator  
Charles Fleddermann, John Gahl, & Donald Shiffler, CO-PIs  
*Pulsed Power & Plasma Science Laboratory*

---

Department of Electrical and Computer Engineering  
University of New Mexico  
Albuquerque, NM 87131

|               |                                     |
|---------------|-------------------------------------|
| Accession For |                                     |
| NTIS CR&I     | <input checked="" type="checkbox"/> |
| DTIC TAB      | <input type="checkbox"/>            |
| Unannounced   | <input type="checkbox"/>            |
| Justification |                                     |
| By            |                                     |
| Distribution  |                                     |
| Date          |                                     |
| DTIC          | Unannounced                         |
| A-1           |                                     |

19950322 162

## Table of Contents

|   |    |
|---|----|
| Section I. Executive Summary .....  | 3  |
| Section II. List of Acquired Equipment .....                                | 4  |
| Section III. Description of Research Program .....                          | 7  |
| Section IV. References .....  | 13 |
| Appendix A. Memorandum requesting changes in original proposed acquisitions | 14 |
| Appendix B. Published journal papers where equipment was used .....         | 22 |

## **I. Executive Summary**

The Pulsed Power & Plasma Science Laboratory at the University of New Mexico (UNM) is pleased to have equipped its laboratory with modern instrumentation in support of its AFOSR-funded program on high power microwave sources. The instrumentation acquired can be broken broadly into three categories:

1. Microwave measurement/calibration (network analyzer and components)
2. Data acquisition (digital oscilloscopes, computers, LabView)
3. High vacuum capabilities (turbo pumps, residual gas analyzer).

This report describes the instrumentation and how it is used in support of the research program.

## **II. List of Acquired Equipment**

The next two pages provides a comprehensive list of equipment that was purchased on this grant, and highlights minor deviations from the AFOSR-approved modified list of equipment (included as Appendix A to this report).

|                                |                              |             |              |
|--------------------------------|------------------------------|-------------|--------------|
| <b>Network Scalar Analyzer</b> |                              |             |              |
| HP 8757XC                      | 20 GHz Coaxial Synthesized   | \$36,225.00 |              |
| W/ Opt. 52B                    | Scalar System                |             |              |
| Opt 002                        | Internal Power Cal           | \$2,250.00  |              |
| Opt 001                        | Fourth Detector Input        | \$1,440.00  |              |
|                                |                              |             | \$39,915.00  |
| HP 85037B                      | Precision Detector           | \$1,665.00  |              |
| HP 85025E                      | AC/DC Detector               | \$1,080.00  |              |
| HP 11679B                      | Detector Cable 200 ft        | \$337.50    |              |
| HP 85025E                      | AC/DC Detector               | \$1,080.00  |              |
| HP 85027E                      | Directional Bridge           | \$2,853.00  |              |
| HP 11679A                      | 3 Detector Cables 25 ft      | \$337.50    |              |
|                                |                              |             | \$7,353.00   |
| HP 85023B                      | Verification Kit for SMA     | \$900.00    |              |
| HP 85023C                      | Verification Kit for Type-N  | \$630.00    |              |
| HP 11636B                      | Power Divider                | \$945.00    |              |
| HP 11667B                      | Power Splitter               | \$963.00    |              |
|                                |                              |             | \$3,438.00   |
|                                |                              |             | \$50,706.00  |
| <b>Oscilloscopes</b>           |                              |             |              |
| TDS 320                        | 3 Digital Oscilloscope       | \$8,456.00  |              |
|                                | 2 Ch, 500 Ms/s with GPIB bus |             |              |
| TDS 350                        | 2 Digital Oscilloscope       | \$7,184.00  |              |
|                                | 2 Ch, 1Gs/s with GPIB bus    |             |              |
|                                | Thermal Printer for Scope    | \$180.56    |              |
| TDS 644A                       | 3 Color Digital Oscilloscope | \$45,145.80 |              |
|                                | 4 Ch, 2 Gs/s                 |             |              |
|                                |                              |             | \$60,966.36  |
| <b>Computers and DAQ</b>       |                              |             |              |
|                                | Mac IIcx with 20 Meg RAM     |             |              |
|                                | and 300 MB Hard Drive        | \$2,987.98  |              |
|                                | Optical Drive                | \$964.40    |              |
|                                | HP 550C Deskwriter Printer   | \$539.97    |              |
|                                | LabView 3.0 for Mac          | \$1,296.75  |              |
|                                | NB-GPIB Board w/cable        | \$539.38    |              |
|                                | Thick Net Adapter            | \$70.38     |              |
|                                | Digital I/O Board            | \$319.50    |              |
|                                | Connecting Block and Cables  | \$216.00    |              |
|                                |                              |             | \$6,934.36   |
|                                | 486DX2 System With 540MB     | \$6,370.00  |              |
|                                | Hard Drive, 16MB RAM         |             |              |
|                                | 21" SVGA Monitor             |             |              |
|                                | Optical Drive, Tape Backup   |             |              |
|                                | Optical discs (10)           | \$329.80    |              |
|                                | LabView3.0 for Windows       | \$1,296.75  |              |
|                                | GPIB Board                   | \$539.37    |              |
|                                | Digital I/O Board            | \$355.50    |              |
|                                | Connecting Block             | \$138.79    |              |
|                                | HP 550C Deskjet Printer      | \$546.44    |              |
|                                |                              |             | \$9,576.65   |
|                                |                              |             | \$16,511.01  |
| <b>Turbo Pumps</b>             |                              |             |              |
|                                | Turbo Pump                   | \$11,175.26 |              |
|                                | Controller for Turbo Pump    | \$5,780.00  |              |
|                                |                              |             | \$16,955.26  |
| <b>Gas Analyzer</b>            |                              |             |              |
|                                | Residual Gas Analyzer        | \$7,500.00  |              |
|                                | Analyzer Head                | \$1,570.00  |              |
|                                |                              |             | \$9,070.00   |
| <b>Total</b>                   |                              |             | \$154,208.63 |

Differences:

- 6 -

Oscilloscopes: TDS 544A did not meet our requirements  
therefore, we ordered three TDS 644A's.

Computers and DAQ:

Did not get DAQ software - used other funds  
to buy Quatro Pro and Paradox Software

Used other funds to buy Ethernet cards (\$150)

Upgraded to 21" Monitor for 486 system

### III. Description of Research Program

The present AFOSR-funded grant on high power microwave sources has three research components:

1. High efficiency vacuum backward-wave oscillators
2. Long pulse vacuum and plasma-filled backward-wave oscillators
3. Ferroelectric cathodes for high power microwave sources.

The microwave measurement/calibration equipment is used on the two backward-wave oscillator (BWO) experiments, the data acquisition is used on all three components of the research program, and the high vacuum equipment is used on the long pulse BWO and on the ferroelectric cathode experiments.

In order to better describe the instrumentation, it would be useful to display photographs of the three experiments, and photographs of some of the acquired equipment.

#### Sinus-6 experiments

The study of high efficiency vacuum BWOs is performed on the Sinus-6 experiment (Fig. 1). This experiment uses LabView 3.0 to acquire and process the data that is taken with the digital oscilloscopes. In addition, the network analyzer is used to calibrate all of the microwave diagnostics and is used as a local oscillator to mix with the generated microwaves in a heterodyne scheme to measure frequency (Figs. 2-3).

These instruments were used to acquire and analyze the data that was used in a recent publication by our group.<sup>1</sup> It is essential to state that the data and understanding presented in this paper would not have been possible without the updated equipment.

#### Long pulse BWO experiments

The study of long pulse vacuum and plasma-filled backward-wave oscillators is performed using a modified PI-110A electron beam accelerator (Fig. 4, top).

This experiment utilizes the data acquisition instrumentation. In addition, it will use the turbo pump and the gas analyzer when it operates at higher power levels than the present time.



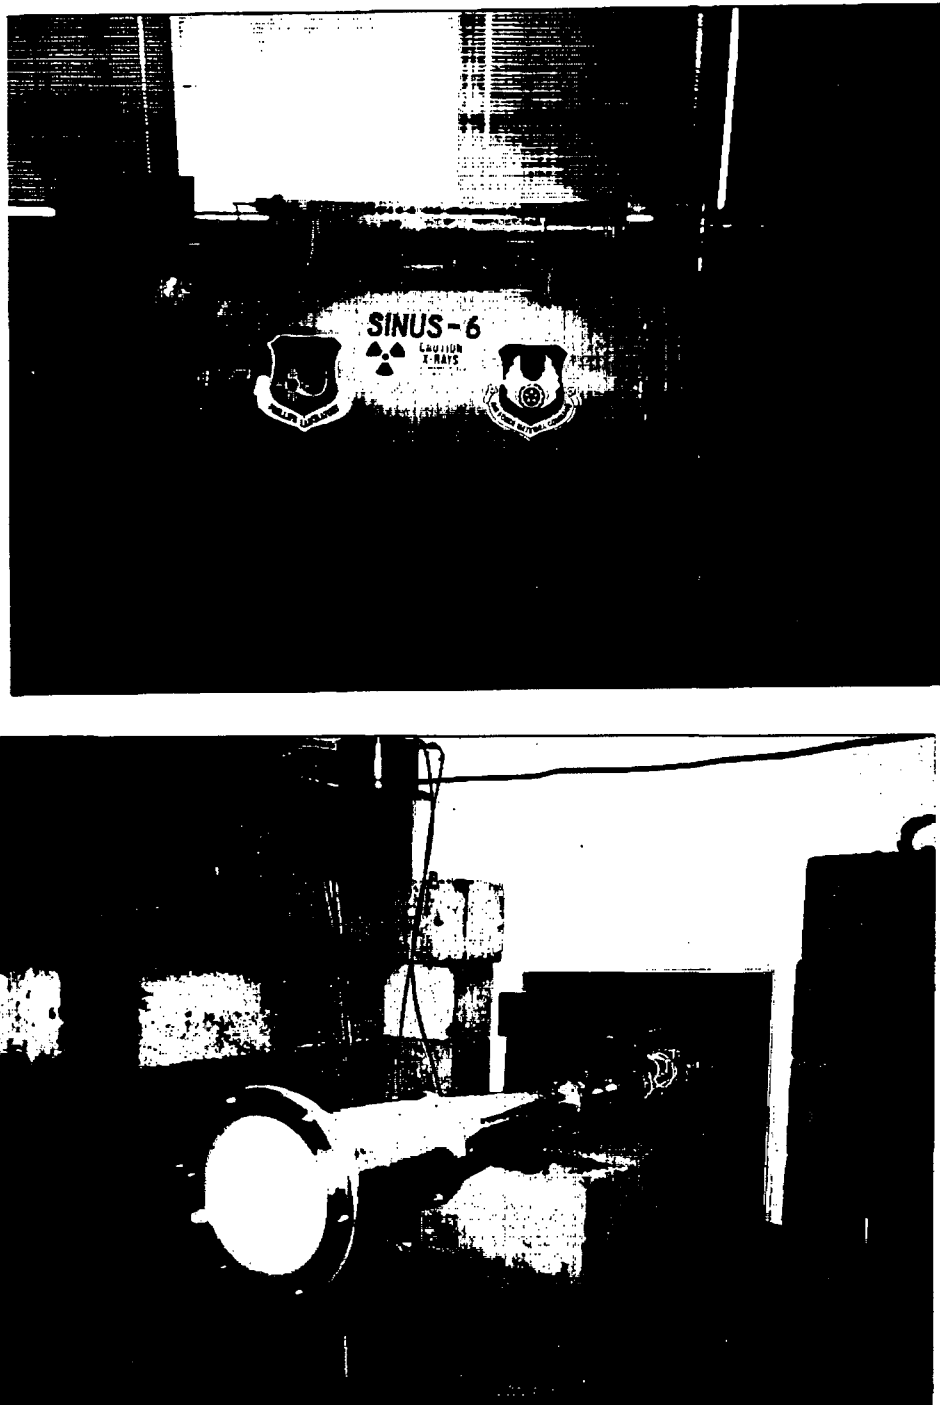


FIG. 1. Photograph of Sinus-6 repetitively-pulsed electron beam accelerator (top) and output of BWO microwave source (bottom).

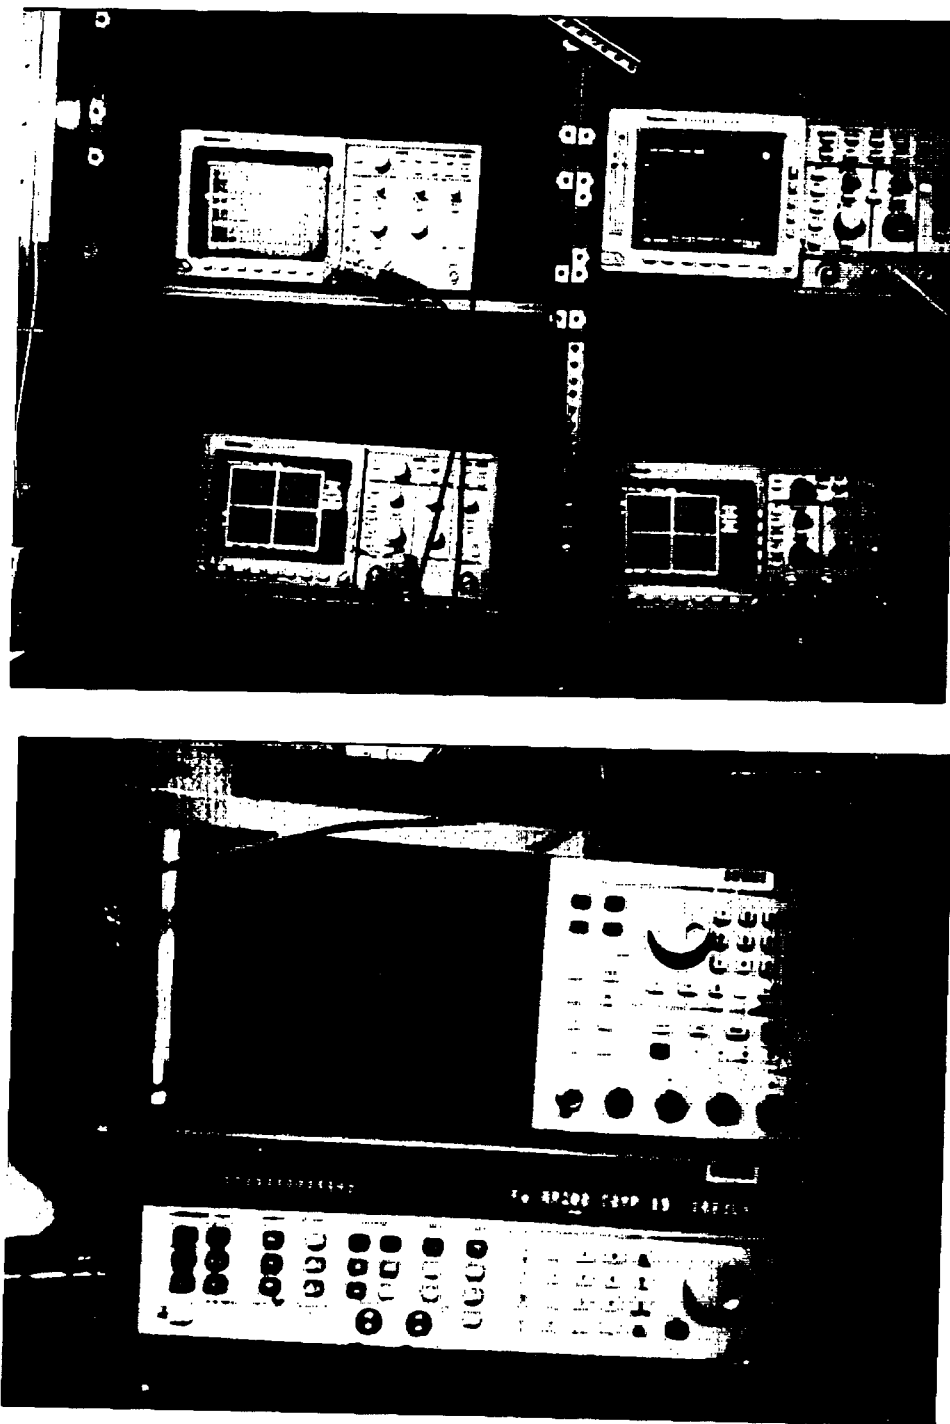


FIG. 2. Array of four digital oscilloscopes (top) and network analyzer (bottom).



FIG. 3. Photograph of screen room showing the computer, digital oscilloscopes, and network analyzer (top). Doctoral candidate Larald Moreland analyzing a shot using LabView (bottom).

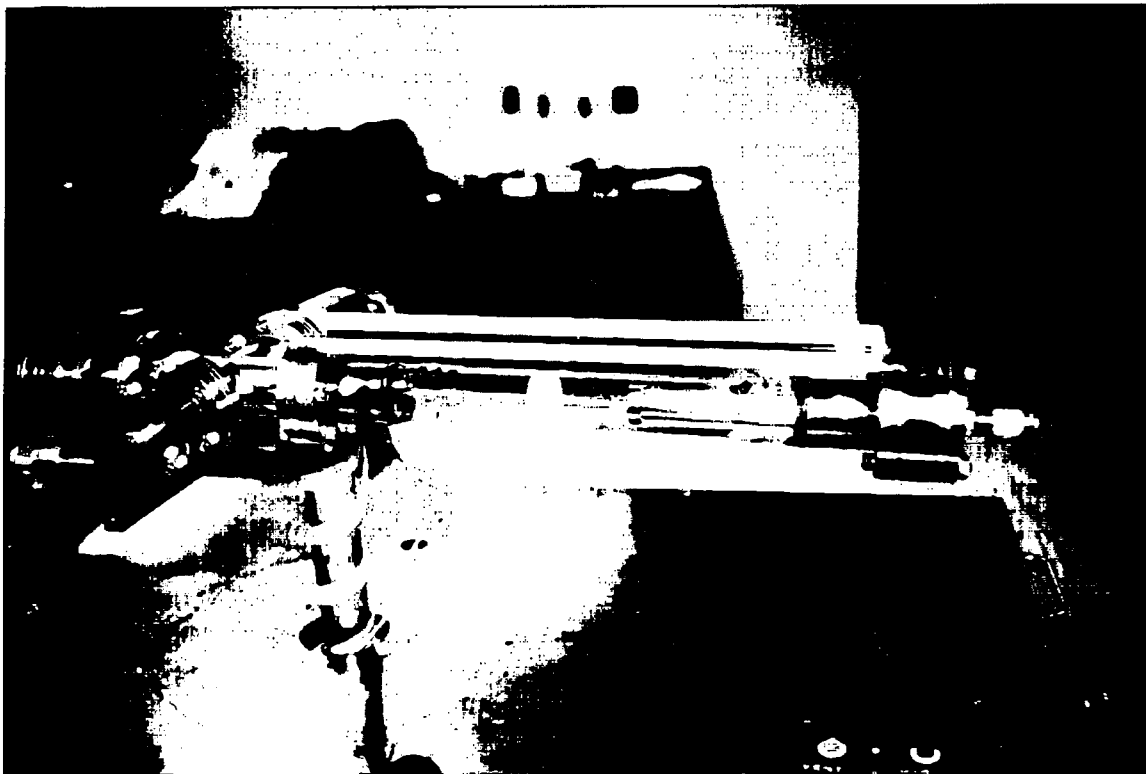
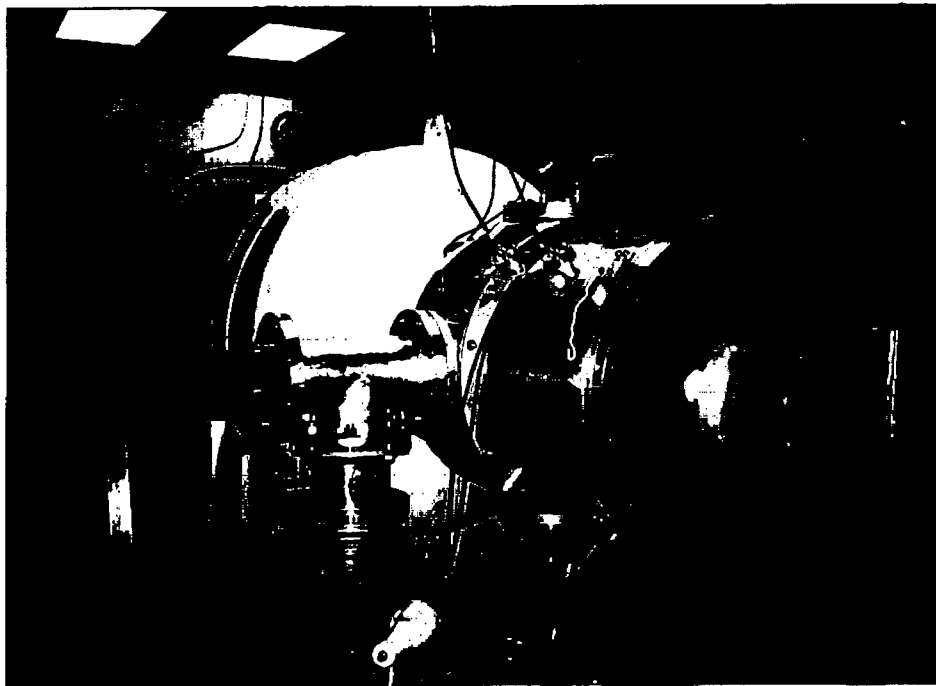


FIG. 4. Photograph of long pulse BWO (top) and ferroelectric cathode test stand (bottom).

### Ferroelectric cathode devevelopment

This experiment utilizes the high vacuum equipment as well as the data acquisition equipment. The ferroelectric cathode test stand is shown in Fig. 4, bottom. The results published in a recent paper<sup>2</sup> used the data acquisition equipment. The residual gas analyzer will be of particular use to this experiment since it will look for evidence of neutrals and plasmas emanating from the cathode periphery. It is important to document whether the ferroelectric electron emission mechanism is accompanied by plasma-based effects.

#### IV. References

1. L. D. Moreland, E. Schamiloglu, R. W. Lemke, S. D. Korovin, V. V. Rostov, A. M. Roitman, K. J. Hendricks, and T. A. Spencer, "Efficiency Enhancement of High Power Vacuum BWO's Using Nonuniform Slow Wave Structures," IEEE Trans. Plasma Sci. **22**, 554 (1994).
2. T. C. Cavazos, W. L. Wilbanks, C. B. Fleddermann, and D. A. Shiffler, "Repeatable electron emission from (Pb,La)(Zr,Ti)O<sub>3</sub> ferroelectric cathodes using direct-current reset," Appl. Phys. Lett. **65**, 2612 (1994).